



Technical Data	
Technology	Direct Reading
Samples/reagents preheating	Yes
Sample capacity and number of reagents	a) Samples 60 positions dedicated to samples/Reagents 27 positions x 27mL each, including stock & diluents b) Samples 70 positions dedicated to samples/Reagents 17 positions x 27mL each, including stock & diluents c) Samples 75 positions dedicated to samples/Reagents 12 positions x 27mL each, including stock & diluents
Test hour	Up to 200 (Single reagent)/120-150 (dual reagent)
Dosing syringe (sample & reagents)	368 microliters syringe with 0.14 µl resolution; Zero automatic setting; Accuracy +/- 0.5% from 2 to 350 uL
Stock solutions on reagent tray	Yes, working calibrants and QC diluted from stocks
Diluents position	On refrigerated reagent tray,
Refrigerated reagent tray	Yes standard
Reagent & Sample level sensor	Yes
Number of reaction cuvettes	80 reaction microcuvettes reusable after washing and QC check, incubation temperature programmable +/- 0.1 °C.
Optical path length (mm)	6.0mm
Reaction plate temperature	37° to 50°C adjustable +/-0.1°C
Incubator type	Thermoelectric
Flow cell type	Bionex ® washable, wash station included
Main Detector	Colorimetric, temperature controlled; halogen lamp extended UV emission; automated zero settings; accuracy +/- 1% from 0 to 2.5 O.D.; linearity better than 0.5%; noise < +/- 2m Abs. At 340 nm 2.5 O.D..
Detector techn./Numb. of Wavelengths	Interferential Filters/ 9+blank
Reading methods	End point: mono o bichromatic; End Point differential (Sample blank correction); Kinetic
Communication & software	USB port; Software compatible Windows XP, 7.0, 8.0 & 10
Sample analysis	Work lists stored by the software with possibility to select independent list of parameters per each sample,
Sample ID	Alphanumeric
Random access to samples, calib. Etc.	Yes
Sample addition during run	Yes
Sample & reagent blanking	Yes
Working Calibrant dilution	Yes, from stock solution located in the refrigerated tray
Pre run sample dilution	Yes
Post run sample dilution	Yes, automated dilution and rerun of off scale samples
Multilevel QC & Closed loop	Up to 5 QC levels, with closed loop control (QC check & pre programmed actions in case of QC and or Spike recovery failure)
QC database and QC chart	Yes
Automated spike & recovery check	Yes
Automated calibrations; calibration fits linear, polynomial, etc.	Yes; up to 16 calibrants
Calibration correction	Yes; enable disable calibrants change calibration fit
Calibration QC check & Calibration repeat	Yes, if correlation lower than set value option for calibration repeat
Reagent Blank OD and Top Cal OD check	Yes, if out of tolerance pre programmed actions
Results correction	Yes, correction by: dilution factor, moisture & weight
Import Work list & export results to LIMS	Yes
Possibility to use multiple diluents (soils analysis, phenols, cyanide etc.)	Yes
Size/Weight	40cmx67cmx60cm(HxDxW)/32Kg
Power Supply	110-240VAC - 50/60Hz Single phase with ground - Fuses 2.0Amp 230VAC, 4.0Amp 115VAC

Subject to change without notice

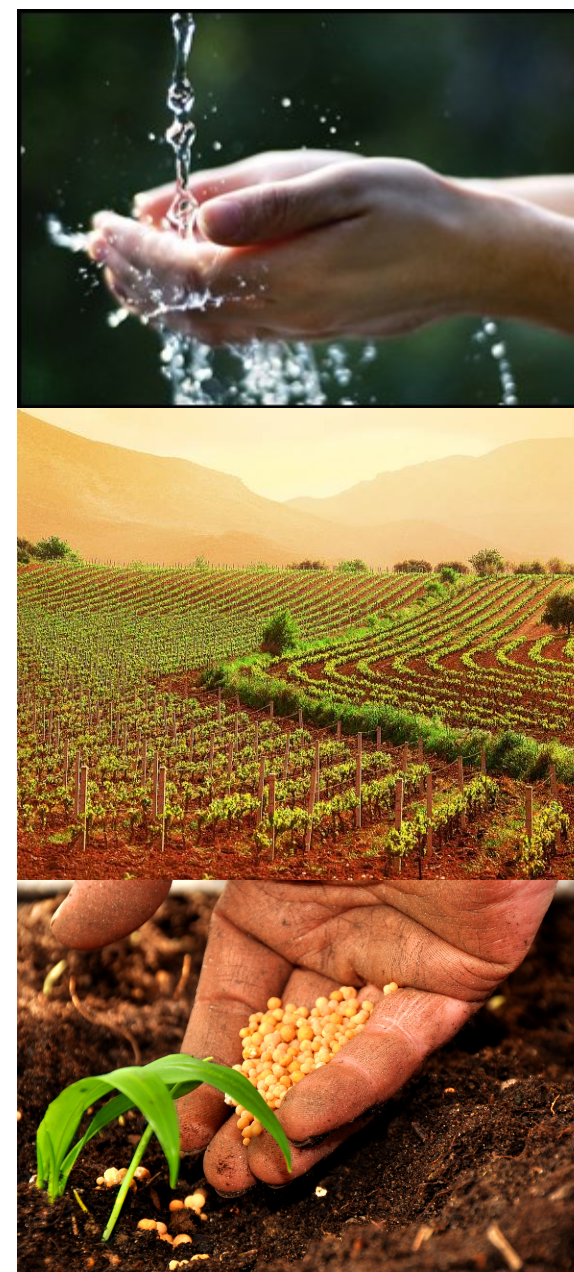

EASYCHEM 200

DIRECT READING DISCRETE
ANALYZER FOR AUTOMATED
CHEMISTRIES

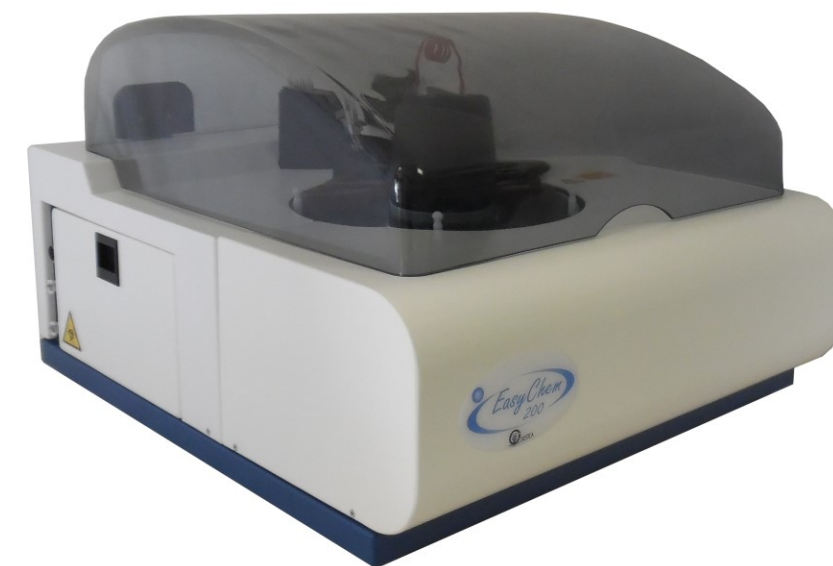

SYSTEAL SpA
Administration and Production: Via Paduni, 2/A - 03012 ANAGNI (FR)
Tel. (+39) 0775.776058 - Fax 0775.772204
e mail: anagni@systea.it
Web site: <http://www.systea.it>

Document ID: EasyChem 200 rev_07E_print (2020024)

EASYCHEM OPERATION PRINCIPLE

A 'work-list' on external PC is created by the operator, containing the samples, their location, their ID code and the determinations required for each sample. Usual combinations of methods can be pre-defined as 'profiles' in the software setup.

The 'work list' includes also calibrants and QC that are automatically diluted from a stock solution in the reaction cuvette. The operator does not need to position any cups other than samples in the work list and in the sample tray.

To start analysis of the work-list or a part of it, the operator has to pass a check-and-confirmation protocol, to establish correct analysis conditions. Selected methods are confirmed, the use of auto-calibration and control samples is set, and the execution is scheduled. Reagent demand and used cuvettes are displayed. Final confirmation starts the execution.

The automatic analyzer starts the execution with a self test procedure, and displays along the execution the actual activity carried out. Analysis results will be reported on the screen just after reading and stored for later printout. Results file can be reprocessed and after reprocessing a results file must be saved with a different name. Stored results documentation for each method is headed by relevant quality data, including the operator ID.



EASYCHEM 200 AUTOMATED DISCRETE ANALYZER

Fully automated analyzer based on **Direct Reading Discrete analysis** technology, sample capacity from 60 up to 75 positions dedicated to samples.

- ✓ Cooled reagents tray with capacity from 12 up to 27 reagents bottles
- ✓ Temperature controlled Reaction tray containing up to 80 reaction cuvettes, washable & reusable after QC check
- ✓ Colorimetric detector including 9 position filter wheel for automatic wavelength selection
- ✓ Pre or post run sample autodilution

The screenshot displays the EASYCHEM 200 software interface. The 'General' tab shows the method name 'Method1', code 'M1', instrument 'Easychem 200', and measuring unit 'mg/l'. The 'Timings and Volumes' tab shows sample volume '100 ul', position 'R1', volume '0', and Nmix '3'. The 'Default Sample Predilution' section shows predilution mode 'Off', predilution % '100', and predilution multiplier '1.0'.

- ✓ Samples throughput: up to 200 test per hour

Water Wastewater methods

ALKALINITY AS CaCO_3

AMMONIA AS N-NH_3

BORON AS B(III)

CALCIUM AS Ca^{2+}

CHLORIDE AS Cl^-

CHLORINE FREE AS Cl_2

CHLORINE TOTAL AS Cl_2

CHROMIUM DISSOLVED AS Cr^{6+}

COLOR AS PT/CO SCALE

COPPER DISSOLVED AS $\text{Cu}^{(\text{I+II})}$

CYANIDE* AS CN^-

FLUORIDE* AS F^-

HARDNESS AS CaCO_3

HYDRAZINE AS NH_2NH_2

IRON DISSOLVED AS $\text{Fe}^{(\text{II+III})}$

LEAD DISSOLVED AS Pb^{2+}

MAGNESIUM AS Mg^{2+}

MANGANESE DISSOLVED AS Mn^{2+}

MONOCHLORAMINE AS NH_2Cl

NICKEL DISSOLVED AS Ni^{2+}

NITRATE AS N-NO_3

NITRATE+NITRITE AS NO_x

NITRITE AS N-NO_2

NITROGEN TOTAL * AS N-NO_3

NITROGEN TKN* AS N-NH_3

ORTHOPHOSPHATE AS P-PO_4

PHENOLICS*AS $\text{C}_6\text{H}_5\text{OH}$

PHOSPHORUS TKP* AS P-PO_4

PHOSPHORUS TOTAL * AS P-PO_4

SILICA AS Si

SULPHATE AS SO_4^{2-}

SULPHIDE AS S^{2-}

UREA AS NH_2CONH_2

ZINC DISSOLVED AS Zn^{2+}

* External sample

pre-treatment required

Soils, plants, feeds and fertilizers*

ALKALINITY - CaCO_3

AMMONIA CaCl_2 -EXTRACT. - N-NH_3

AMMONIA KCl -EXTRACT. - N-NH_3

BORON CaCl_2 -EXTRACTABLE - $\text{B}^{(\text{III})}$

CALCIUM - $\text{Ca}^{(\text{II})}$

CHLORIDE WATER-EXTRACTABLE - Cl^-

COPPERACID-EXTRACTABLE - $\text{Cu}^{(\text{I+II})}$

IRON ACID-EXTRACTABLE - $\text{Fe}^{(\text{II+III})}$

MAGNESIUM - $\text{Mg}^{(\text{II})}$

NITRATE CaCl_2 -EXTRACT. AS N-NO_3

NITRATE KCl -EXTRACT. - N-NO_3

NITRATE WATER-EXTRACT. - N-NO_3

NITROGEN TOTAL KJELDAHL - N-NH_3

PHOSPHORUS ACID-EXTRACT. - P-PO_4

PHOSPHORUS AVAIL.-BRAY - P-PO_4

PHOSPHORUS CaCl_2 -EXTRACT. - P-PO_4

PHOSPHORUS COLWELL-EXTR. - P-PO_4

PHOSPHORUS KJELDAHL - P-PO_4

PHOSPHORUS OLSEN-EXTRACT. - P-PO_4

PHOSPHORUS SORPTION - P-PO_4

PROTEIN TOTAL

SILICON ACID-EXTRACTABLE - Si

SILICON CaCl_2 -EXTRACTABLE - Si

SULPHATE CaCl_2 -EXTRACT.- SO_4^{2-}

ZINC ACID-EXTRACTABLE - $\text{Zn}^{(\text{II})}$

NOTE

Method list includes only the most common methods and it is under continuous development.

For any method not included in the list please contact our application laboratory to check method availability

* External sample pre-treatment required

ADVANTAGES AND BENEFITS

- **Easy to use:** no specific experience or training required.
- **Flexibility:** individual parameters list selectable on each sample, pre or post run sample autodilution, working standard autodilution from a stock standard.
- **Low reagents consumption:** only a few microliters of reagents per analysis.
- **Low running costs:** nearly no consumables, low reagents and disposable costs.
- **Immediate start up:** no time waste or problems to reach hydraulic equilibrium.
- **Immediate shut down:** no washing procedure required.
- **Windows based Software:** easy to use and to learn; short training, specifically designed for chemists.
- **QC control:** up to five level of real time QC can be used, QC results are automatically stored and plotted in a quality control chart.
- **QC actions:** in case of QC out of tolerance the analyzer can stop the run or simply inform the operator leaving trace of malfunction storing the QC out of tolerance.
- **Data reprocessing** allows to check and reprocess the results file, including or deleting data treatment.

