






# EasySlim

## CATALOG

### Implantline

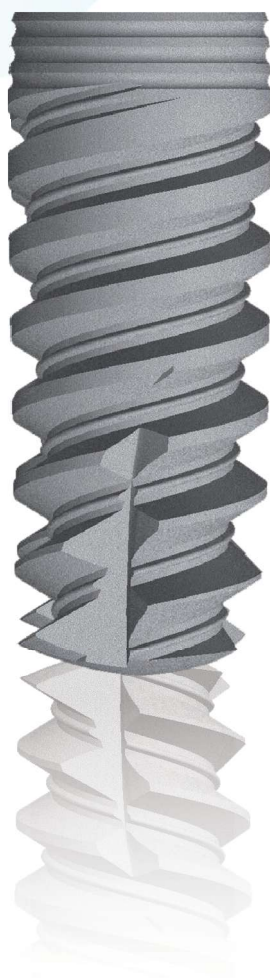

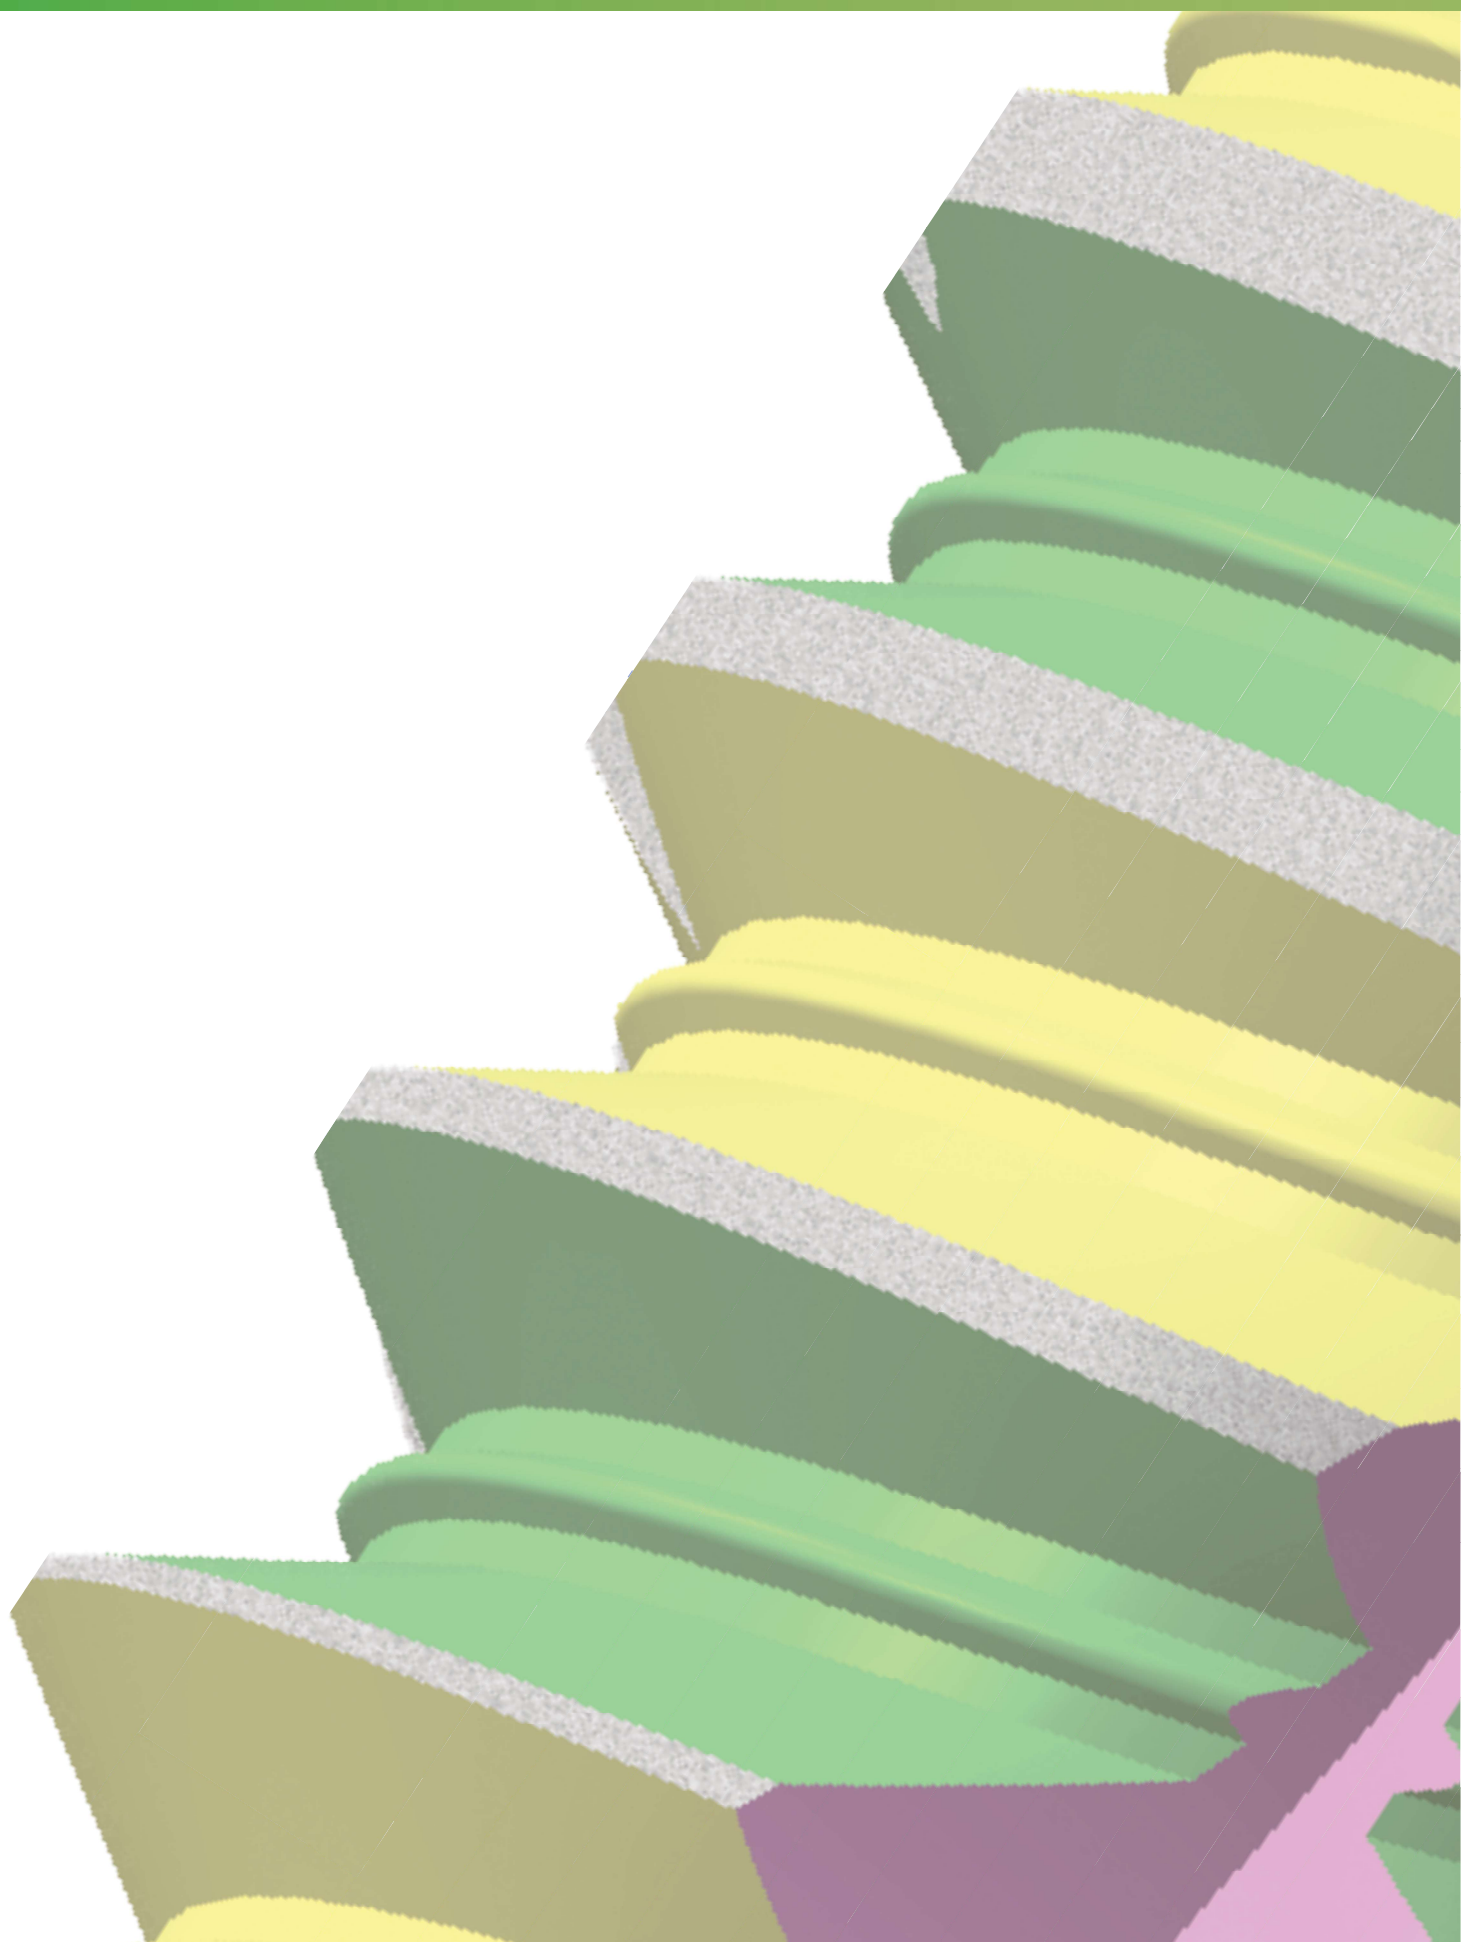


# Contents



The range	4
Surgical sequence	6
The stops cutter	7
Chirurgical tray	8-9
<b>Description prosthetic</b>	
Healing	10
The foot print	11
Prosthetic components	12
Overdenture	14
OTEquantor	15
MUA angled abutments	16
TechnicalCADCAM	18
Screws	21

# The range

## Plant

Implant	Length	Code Art.	Size			
			A	B	C	D
 Ø 3,3	10 mm	1033ES	Ø 3,8	Ø 3,1	Ø 1,85	Ø 3,5
	11,5 mm	1133ES	Ø 3,8	Ø 3,0	Ø 1,70	Ø 3,5
	13 mm	1333ES	Ø 3,8	Ø 2,95	Ø 1,55	Ø 3,5
	16 mm	1633ES	Ø 3,8	Ø 2,85	Ø 1,25	Ø 3,5
 Ø 3,8	8 mm	0838ES	Ø 3,9	Ø 3,0	Ø 2,60	Ø 3,5
	10 mm	1038ES	Ø 3,9	Ø 3,70	Ø 2,35	Ø 3,5
	11,5 mm	1138ES	Ø 3,9	Ø 3,60	Ø 2,20	Ø 3,5
	13 mm	1338ES	Ø 3,9	Ø 3,50	Ø 2,05	Ø 3,5
	16 mm	1638ES	Ø 3,9	Ø 3,40	Ø 1,95	Ø 3,5
 Ø 4,2	6 mm	0642ES	Ø 4,3	Ø 4,25	Ø 3,10	Ø 3,5
	8 mm	0842ES	Ø 4,3	Ø 4,15	Ø 2,85	Ø 3,5
	10 mm	1042ES	Ø 4,3	Ø 4,05	Ø 2,65	Ø 3,5
	11,5 mm	1142ES	Ø 4,3	Ø 4,00	Ø 2,50	Ø 3,5
	13 mm	1342ES	Ø 4,3	Ø 3,90	Ø 2,35	Ø 3,5
	16 mm	1642ES	Ø 4,3	Ø 3,80	Ø 2,05	Ø 3,5
 Ø 5,0	6 mm	0650ES	Ø 5,0	Ø 4,95	Ø 3,90	Ø 3,5
	8 mm	0850ES	Ø 5,0	Ø 4,85	Ø 3,65	Ø 3,5
	10 mm	1050ES	Ø 5,0	Ø 4,75	Ø 3,45	Ø 3,5
	11,5 mm	1150ES	Ø 5,0	Ø 4,70	Ø 3,30	Ø 3,5
	13 mm	1350ES	Ø 5,0	Ø 4,65	Ø 3,15	Ø 3,5
	16 mm	1650ES	Ø 5,0	Ø 4,54	Ø 2,80	Ø 3,5
 Ø 6,0	6 mm	0660ES	Ø 6,0	Ø 5,95	Ø 4,90	Ø 3,5
	8 mm	0860ES	Ø 6,0	Ø 5,85	Ø 4,65	Ø 3,5
	10 mm	1060ES	Ø 6,0	Ø 5,75	Ø 4,45	Ø 3,5
	11,5 mm	1160ES	Ø 6,0	Ø 5,70	Ø 4,30	Ø 3,5
	13 mm	1360ES	Ø 6,0	Ø 5,65	Ø 4,15	Ø 3,5
	16 mm	1660ES	Ø 6,0	Ø 5,54	Ø 3,80	Ø 3,5



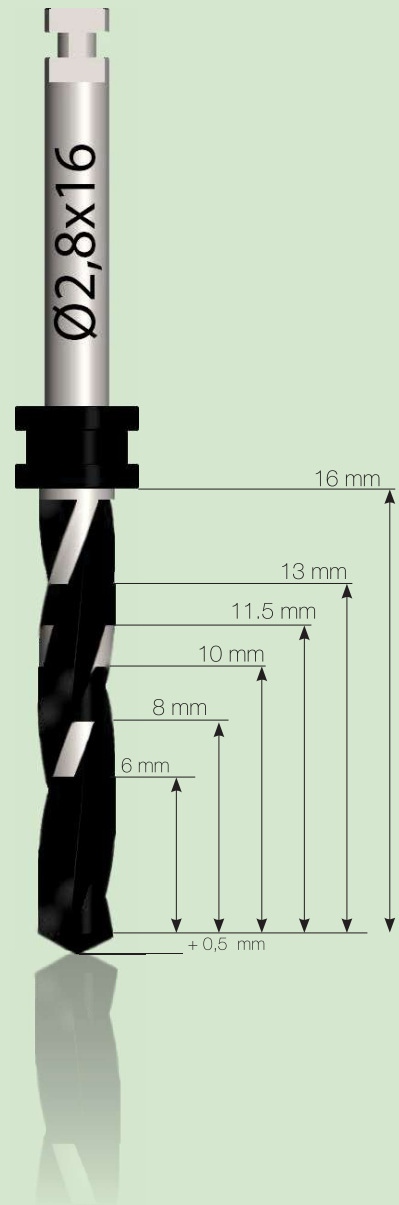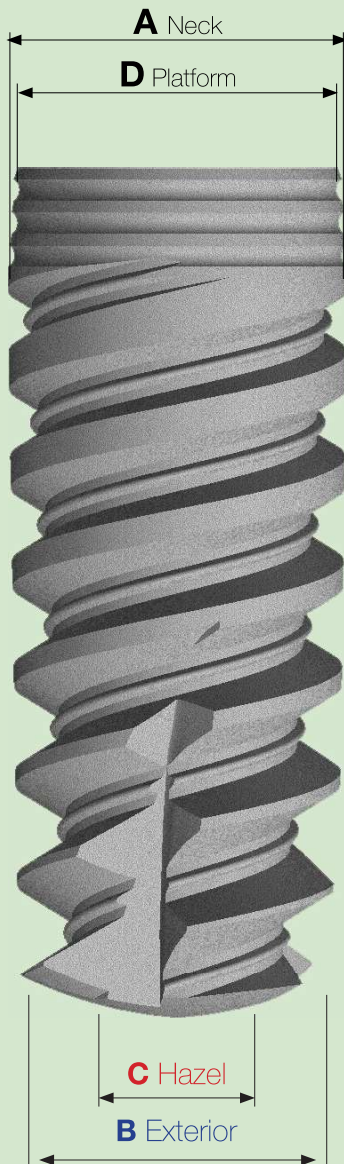

#### SCREW CAP



Made of Gr.5 titanium, it is provided in every implant package. Can be used manually with the driver (e.g. 1.3 mm. recommended closure Torque 15/20 Ncm.)

# The surgical sequence



PLANT Ø 3.3



- Step 1:** Lanceolate cutter  
**Step 2:** drill Ø 2,0 - Ø 2,8 the implant length  
**Step 3:** drill Ø 3,2 1/3 the implant length  
**Step 4:** For **DI** drill Ø 3,2 la 2/3 implant length

N° turns/min.: 1200  
 N° turns/min.: 900  
 N° turns/min.: 900  
 N° turns/min.: 900



IPLANT Ø 3.8




- Step 1:** Lanceolate cutter  
**Step 2:** drill Ø 2,0 - Ø 2,8 the implant length  
**Step 3:** drill Ø 3,2 2/3 the implant length  
**Step 4:** For **DI** drill Ø 3,7 1/3 the implant length

N° turns/min.: 1200  
 N° turns/min.: 900  
 N° turns/min.: 900  
 N° turns/min.: 900



PLANT Ø 4.2

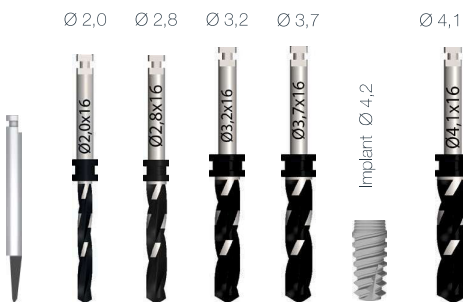


- Step 1:** Lanceolate cutter  
**Step 2:** drill Ø 2,0 e Ø 2,8 the implant length  
**Step 3:** drill Ø 3,2 - Ø 3,7 2/3 the implant length  
**Step 4:** For **DI** drill Ø 4,1 1/3 the implant length

N° turns/min.: 1200  
 N° turns/min.: 900  
 N° turns/min.: 900  
 N° turns/min.: 900



PLANT Ø 5.0

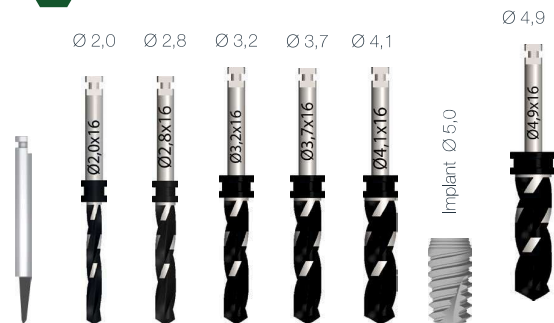


- Step 1:** Lanceolate cutter  
**Step 2:** Ø 2,8 , Ø 2,8 e Ø 3,2 the implant length  
**Step 3:** drill Ø 3,7- Ø 4,1 a 2/3 the implant length  
**Step 4:** For **DI** drill Ø 4,9 1/3 the implant length

N° turns/min.: 1200  
 N° turns/min.: 900  
 N° turns/min.: 900  
 N° turns/min.: 900



PLANT Ø 6.0

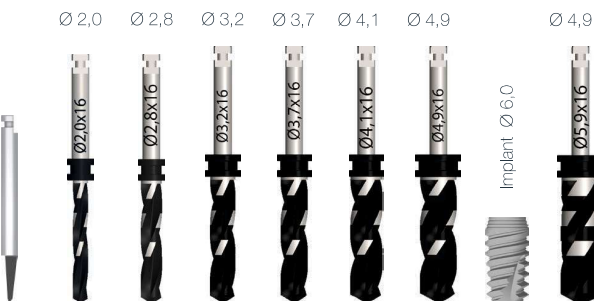


- Step 1:** Lanceolate cutter  
**Step 2:** Ø 2,8 , Ø 2,8 e Ø 3,2 the plant length  
**Step 3:** drill Ø 3,7- Ø 4,1- 4,9 la 2/3 the implant length  
**Step 4:** For **DI** drill Ø 5,9 1/3 the implant length

N° turns/min.: 1200  
 N° turns/min.: 900  
 N° turns/min.: 900  
 N° turns/min.: 900

# The Stopscutter

The stops for the Ø 2,0-Ø 2,9 cutter

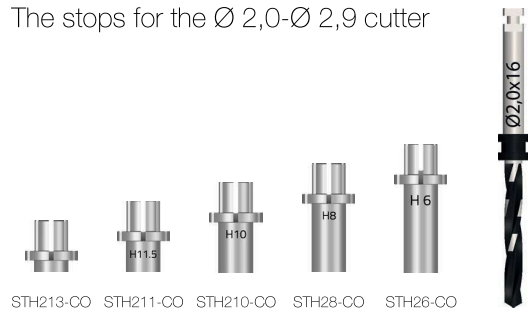

The stops for the Ø 3,1-Ø 3,9 cutter



The stops for the Ø 4,0-Ø 4,9 cutter




## The stop cutters







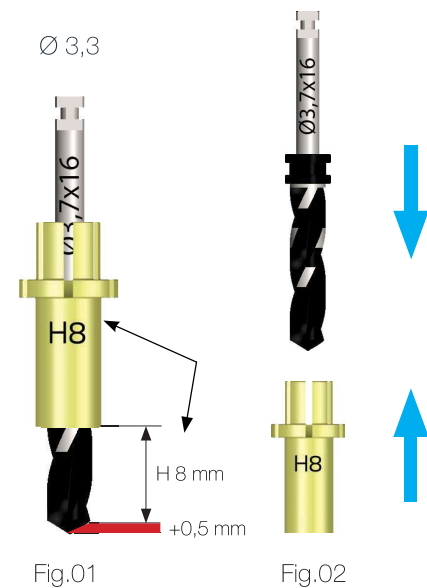














They are made of Ti Gr5, and their use is expected on all Conical Grade cutters. On the body of the cutter stop is laser engraved the depth that the stop allows to reach (Fig.01). The cutter stop is attached to the cutter through a mechanical seal. Orienting the cut cylindrical part upward causes the cutter tip to engage downward, so the cutter and the stop are assembled (Fig.02).







## The cutter stop box

The cutter stop box is designed to make it easy to apply and remove the stop from the cutter, without the need to touch the accessories with your hands.



# Chirurgicaltray

	Article Size	code	Tray KIT03
	Lanceolata	FBCO01	YES
	Extension Drill	EDCO01	YES
	Drill Ø 2,0 L16	TDEI216S	YES
	Drill Imp. Ø 2,8 L16	TDEI2816S	YES
	Drill Imp. Ø 3,2 L16	TDCO3216S	Optional
	Drill Imp. Ø 3,7 L16	TDCO3716S	YES
	Drill Imp. Ø 4,1 L16	TDCO4116S	YES
	Drill Imp. Ø 4,9 L16	TDCO4916	Optional
	Drill Imp. Ø 5,9 L16	TDCO5916	YES
	Es 1,3 L 9	MNCO13S	Optional
	Es 1,3 L 10	MNCO13M	Optional
	Es 1,3 L 13	MNCO13L	Optional
	Es 1,3 L 13	DRCO13S	Optional
	Es 1,3 L 17	DRCO13M	YES
	Es 1,3 L 23	DRCO13L	Optional
	L 8 per Imp	WMNES24S	Optional
	L 11 per Imp	WMNES24M	YES
	L 16 per Imp	WMNES24L	Optional
	L 13 per Imp	DRES24S	Optional
	L 17 per Imp	DRES24M	YES
	L 23 per Imp	DRES24L	Optional

	Article Size	code	Tray KIT03
	Ø 2,0-Ø 2,7	PRCO01	Optional
	Ø 3,2-Ø 3,7	PRCO02	Optional
	-	ADWHK01	Optional
	15-35 Ncm	CRIC01	Optional
	25-55 Ncm	CRIC02	Optional
	Rigida	CRIC03	YES

# Thehealing

## Healing abutments




**Easy Slim®** Healing Abutments® are manufactured from medical-purity Titanium Gr5 and are used to condition soft tissues by preparing them To accommodate the temporary or permanent prosthesis.


**Torque:** Tightening to 15÷20 Ncm.

**Packaging:** the package provides only one healing stump.


### Ø 3,8

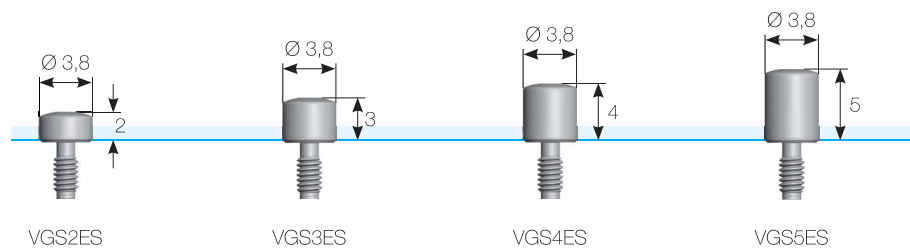


### Ø 4,7

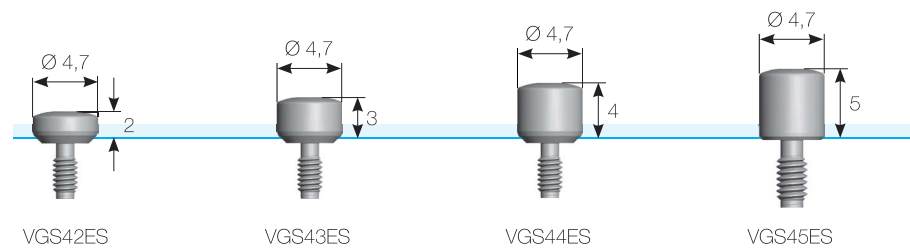


### Ø 5,0

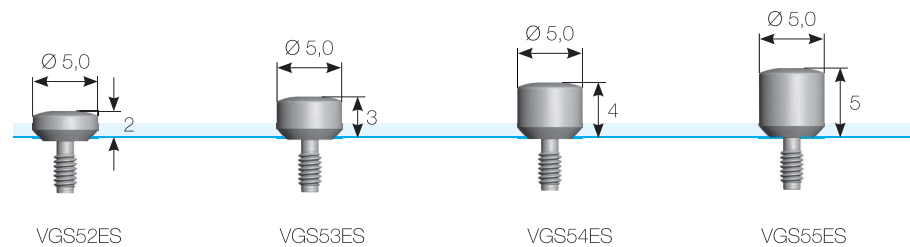

### Ø 6,0

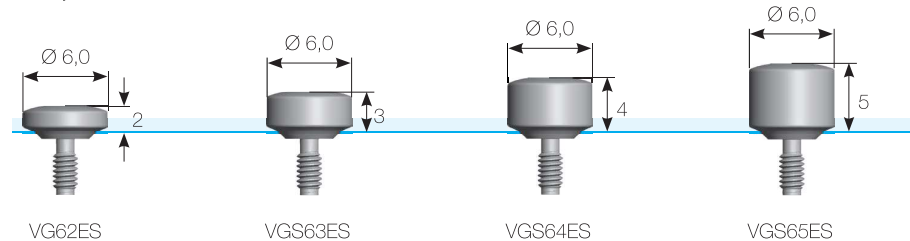

## Peek healing abutments

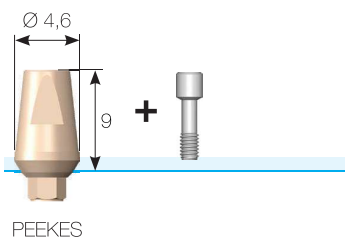


**Easy Slim** Healing Abutments® are made of medical Peek and are used to condition the soft tissues, preparing them to accommodate the temporary or final prosthesis.

**Torque:** Tightening to 20÷25 Ncm.

**Packaging:** the package includes a single peek healing stump plus its prosthetic screw.

## The footprint

### Imprint transfer

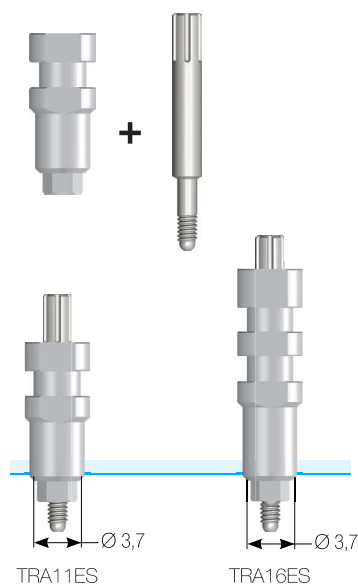

The **Easy Slim** Impression Pick Up® is made of medical-purity Titanium Gr5 and is used to take an impression with an individual spoon.

**Torque:** Tightening to 15 Ncm.

**Packaging:** the package includes one Pick Up and its screw.

### Chalk analogue




Plaster analog, inserted into the Pick Up or Impression Transfer is used to reproduce in plaster the exact projection of the implant.

**Packaging:** the package provides only one Chalk Analog.

ANA16ES

### Pick up

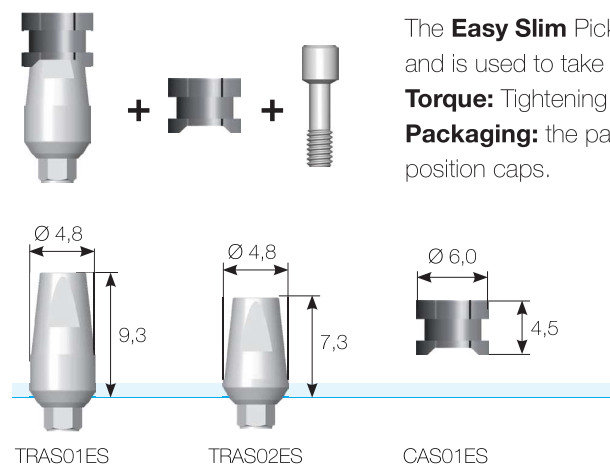


The **Easy Slim** Pick up is made of medical-purity Titanium Gr5 and is used to take an impression with a closed spoon.

**Torque:** Tightening to 15 Ncm.

**Packaging:** the package includes one Transfer its screw and 3 position caps.

# Prosthetic components

## Straight titanium abutments

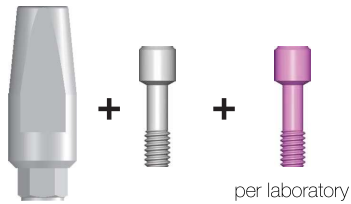


All **Easy Slim** Straight and Angled Titanium Abutments® are manufactured from Gr5 titanium and are used for the fabrication of the final prosthesis.

**Torque:** Tightening to 25÷25 Ncm.


**Packaging:** the package includes a single titanium stump with and the final screw.

## Straight abutments to finish

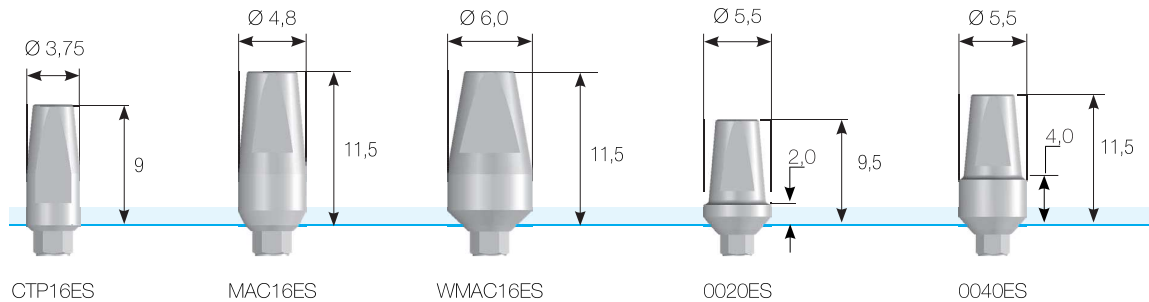


## Shoulder abutments

## Angled abutments

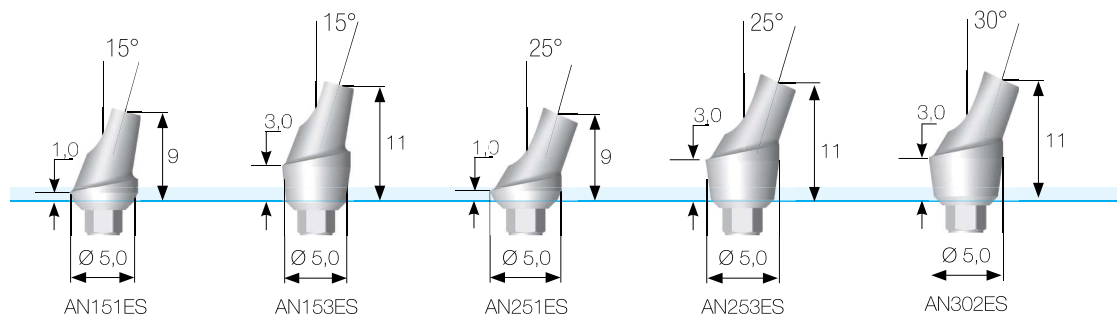



## Calcinable with CoCrMo base




CoCrMo **Easy Slim®** base is molybdenum (CoCrMo). It is free of nickel and beryllium; its fine structure, a product of powder metallurgy processes, prevents deformation of parts after the + processing. An additional advantage of molybdenum in the manufacture of dentures is the stability of the alloy at high temperatures, which facilitates combination with ceramics.

**Melting range °C :** 1350-1450

**Torque:** Tightening to 25 Ncm.


**Packaging:** the package includes a CrCoMo base, a calcinable, and a prosthetic screw.

### With index

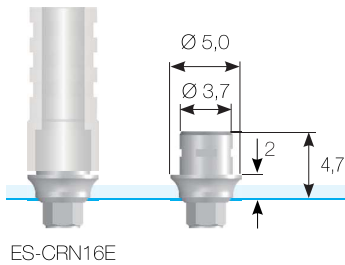


ES-CRN16E

### Rotating

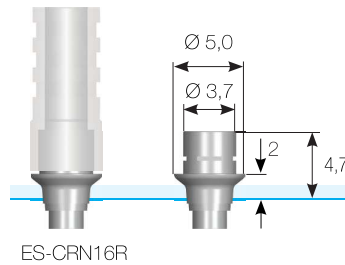

ES-CRN16R

## Calcinable




**Easy Slim®** calcinable abutment

**Melting range °C :** 900 Torque:

Tightening at 25 Ncm.


**Packaging:** the package includes one calcinable and one prosthetic screw.

### with hexagon

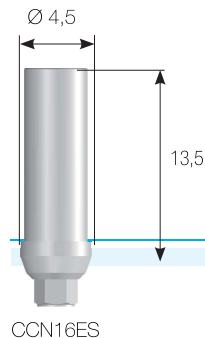

CCN16ES

### without hexagon

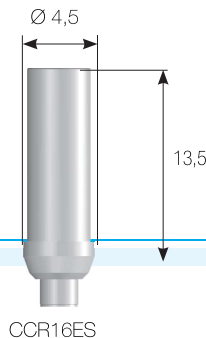

CCR16ES

# Overdenture

## Ball abutment




The **Easy Slim®** Ball abutment is made of Titanium Gr5.

It is used to make removable dentures.


**Torque:** Tightening to 25 Ncm.

**Packaging:** the package includes a Ball Abutment.

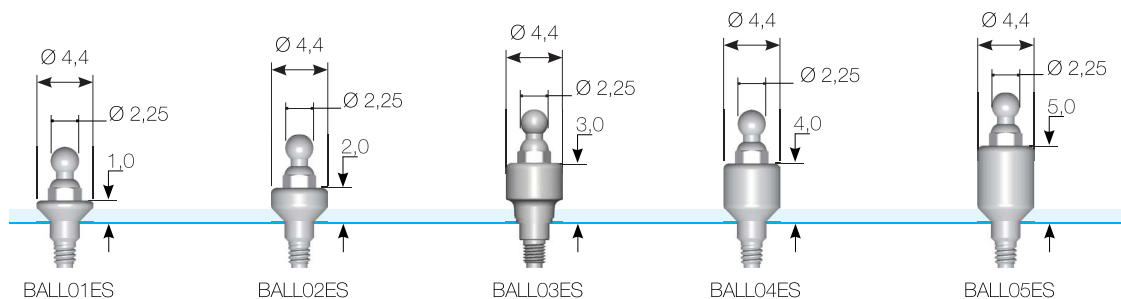

## Ball abutment spare parts

O'Ring



CG-GO01

Kit Package



1 pz.

3 pz.

O'Ring


Package of 5 pcs.



ORCG01

standard seal

O'Ring



CG-GO02

Kit Package



1 pz.

3 pz.

O'Ring

Package of 5 pcs.



ORCG02

soft hold


## Spare parts overdenture

Container




CAOES01

Standard sealing




CA001

Soft seal liners Ø



CN001

Standard sealing



CN002

# OT Equator


## Ot Equator kit



The Ot Equator component is constructed of Gr5 titanium and coated in Tin.

**Torque:** Tightening to 25 Ncm.

**The package includes:** 1 Tin-coated Titanium attachment, 1 stainless steel cap container, 1 protective diskette, 4 assorted caps (1 extra-soft, 1 soft, 1 standard, 1 strong).

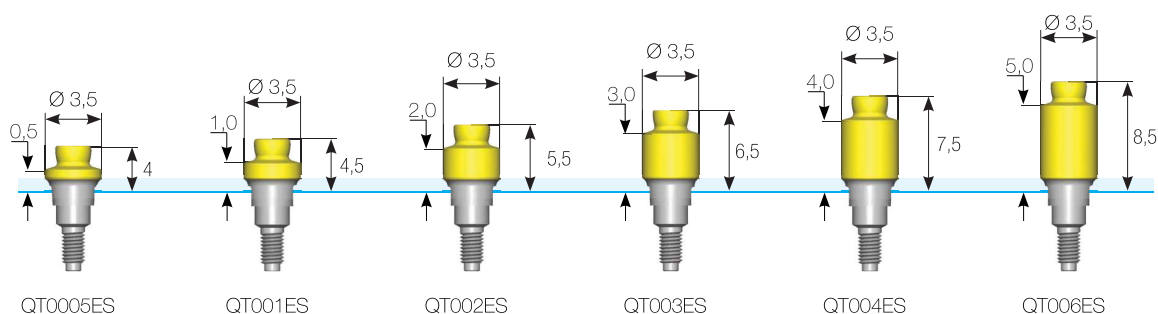

## Overdenture Parts

### Sheaths




CNL4ES

Laboratory




CBST4ES

Standard seal (1.8 kg)




CRS4ES

Soft seal (1.2 kg)



CGE4ES

Extra soft seal (0.6 kg)



CVF4ES


Strong Tightness (2.7 kg)

### Container Ø



ES-C12

### Protective sheathing



GACG001

## Ot Equator laboratory

### Chalk analogue



CGANSF01

Rhein 83  
Ref 144AE. 2 pz

### Individual transfer



Rhein 83  
Ref. 144MTE 2 pz

### Tear-off transfer



Rhein 83  
Ref. 044CAIN 2 pz

### For handpiece



Rhein 83  
Ref. 760CE 1 pz

### For ratchet



Rhein 83  
Ref. 774CHE 1 pz

# MUA **angled** abutments


## Straight Multi Unit Abutment



The straight multi-unit abutment is made of Gr5 titanium and is used for fabricating screw-retained prostheses on multiple elements and in the case of disparallel implants (all on four technique).

**Torque:** Tightening to 25 Ncm.

**Packaging:** the package provides a single component.

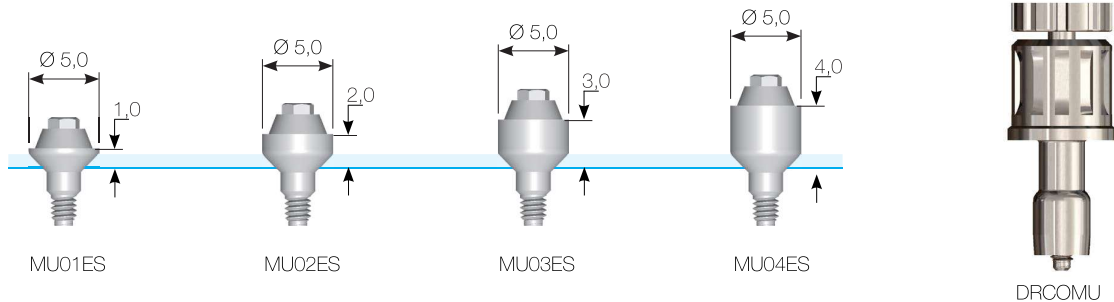

## The Angled Multi Unit Abutments




The angled Multi Unit abutment is constructed from Gr5 titanium and is used for fabricating screw-retained multi-unit prostheses for 17° and 30° angled implants


**Torque:** Tightening to 25 Ncm.

**Packaging:** the package includes the angled connector and its prosthetic screw.

Angolato 17°

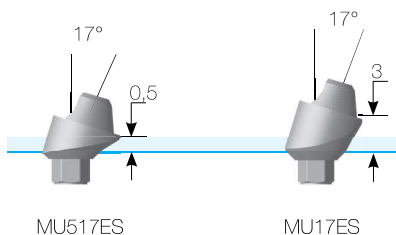

Angolato 30°

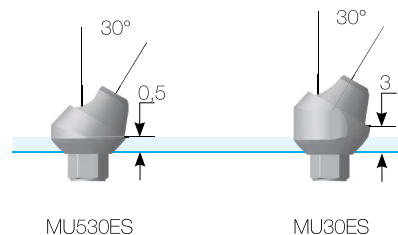

## Cover for straight and angled Multi Unit abutments




The healing screw for straight and angled Multi Unit abutments is constructed of Gr5 titanium and serves to protect the connection cones of the straight connectors and angled connectors.

**Torque:** Tightening to 20 Ncm.

**Packaging:** the package includes a healing cover and its screw.

# MUA abutments

## Titanium abutment

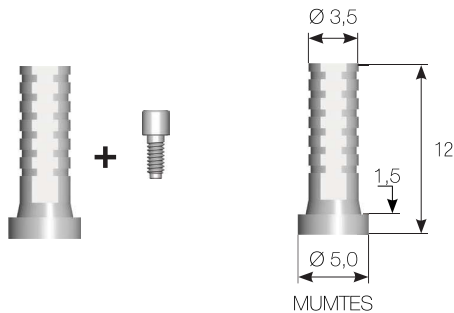


The **Easy Slim®** Straight and Angled Multi Unit Titanium Abutment is manufactured from Gr5 titanium, is used for the fabrication of temporary and/or final prosthesis.

**Torque:** Tightening to 20 Ncm.

**Packaging:** the package includes one titanium abutment with one prosthetic screw.

## Calcinable abutment

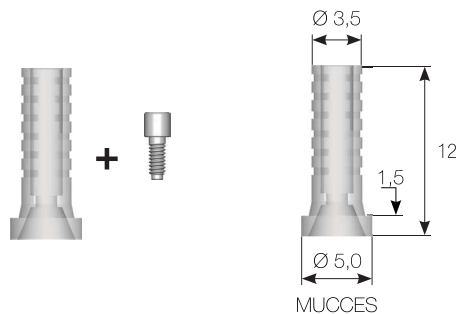


The castable for straight and angled Multi Unit abutments **Easy Slim®** is made of PMMA and is used to cast metal. Melting range °C : 160-175

**Torque:** Tightening to 25 Ncm.

**Packaging:** the package includes one calcinable, one prosthetic screw.

## Imprint transfer

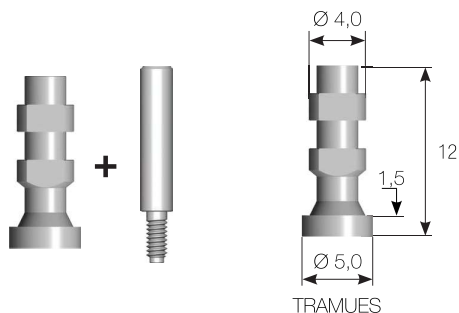

The **Eeasy Slim®** Straight and Angled Multi Unit Abutment Impression Transfer is made of Titanium Gr5 and is used for individual tray impression taking.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package includes one calcinable, one screw.

## Chalk analogue




The plaster analog is the same as that used for the CAD/CAM technique; it is made of Gr5 titanium.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package provides only one analogue.

# TechnicalCADCAM

## Scan Marker by Implant




The Marker is manufactured from a single part of Gr5 titanium.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package includes a Marker and a screw for its tightening CG-VS7818.

## Scan Marker by Implant

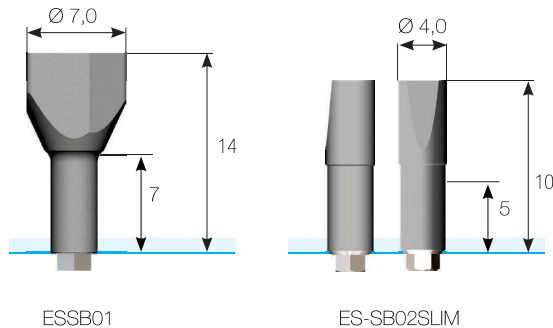


The Marker is manufactured from a single part of Gr5 Titanium.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package includes a Marker and a screw for its tightening CG-VS7818.

## CAD CAM Premilled from cementing

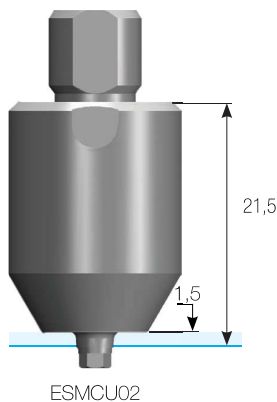

Premilled, are manufactured from Gr5 titanium, a single diameter and height. The Premilled 10 mm diameter is ideal for customized machining on milling machines.

**Torque:** Tightening to 25-30 Ncm.

**Packaging:** the package includes a Premilled and a screw for its tightening.

## Digital analogue for CAD CAM technique




The digital analogue for the CAD CAM technique is made of Gr5 titanium. Its special shape allows its easy positioning in molded models and with remarkable simplicity its anchorage to the model by using a screw (M1,6) that is screwed between the bottom of the model and the bottom of the analog.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package includes an analog with the screw.

# TechnicalCADCAM

## Ti Bonding Base for CAD/CAM Technique




Base bonding Tis are constructed from Gr5 titanium. Base Ti are offered in three different heights to compensate for even deep mucosal paths.

**Torque:** Tightening to 25-30 Ncm.

**Packaging:** the package includes a Digital Ti base and a VS7818 prosthetic screw.


with Index      without Index



ESTBE0

ESTBR0


with Index      without Index



ESTBE2

ESTBR2


with Index      without Index

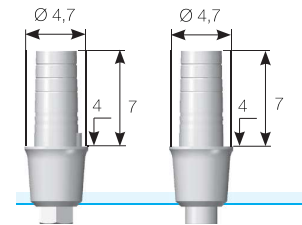

ESTBE4

ESTBR4


with Index      without Index



ESTBSAE0

ESTBSAR0


with Index      without Index



ESTBSAE2

ESTBSAR2

with Index      without Index

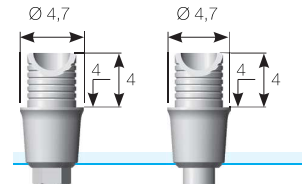


ESTBSAE4

ESTBSAR4

# Technical CAD CAM MUA

## MUA Scan Marker

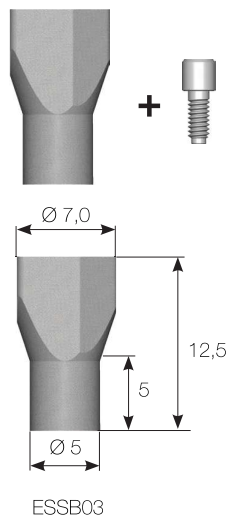


The MUA Abutment Marker is fabricated in two parts: Gr5 Titanium core that is assembled to a scannable Peek part.

The Marker is constructed from a single size.

**Torque:** Tightening to 15-20 Ncm.

**Packaging:** the package includes a Marker and a screw for its tightening CG-VS3414.

## Digital Ti base MUA

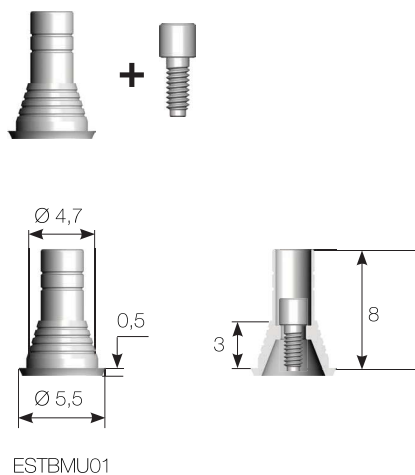


The basic Ti for MUA is constructed of Gr5 titanium.

**Torque:** Tightening to 25-30 Ncm.

**Packaging:** the package includes a Digital Ti base and a CG-VS3414 prosthetic screw.

## Digital analogue for CAD CAM technique

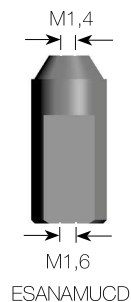

The MUA digital analogue for the CAD CAM technique is made of Gr5 titanium. Its special shape allows its easy placement in printed models and with remarkable simplicity its anchoring to the model by using a screw (M1,6) that is screwed between the bottom of the model and the bottom of the analog.

**Torque:** Tightening to 15-20 Ncm.


**Packaging:** the package includes an analog with the screw.



# Screws

## Standard denture screws

### Per abutment

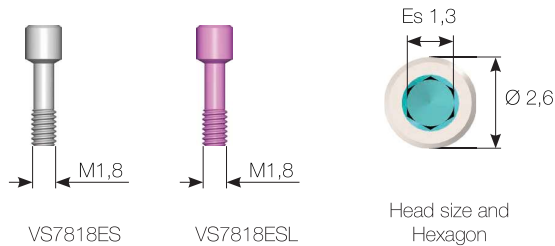


The prosthetic screws are made of Gr5 titanium and are of two types. The **Easy Slim** provides a fuchsia-colored screw for laboratory use and a machined gray screw for patient-only use.

**Torque:** Tightening to 25-30 Ncm.

**Packaging:** packages include 5 pcs.

## Angled denture screws

### For abutment




The prosthetic screw for the angled technique is cotruded from Gr5 titanium.

**Torque:** Tightening to 20-25 Ncm.

**Packaging:** packages include 5 pcs.

## For Pick Up - plant

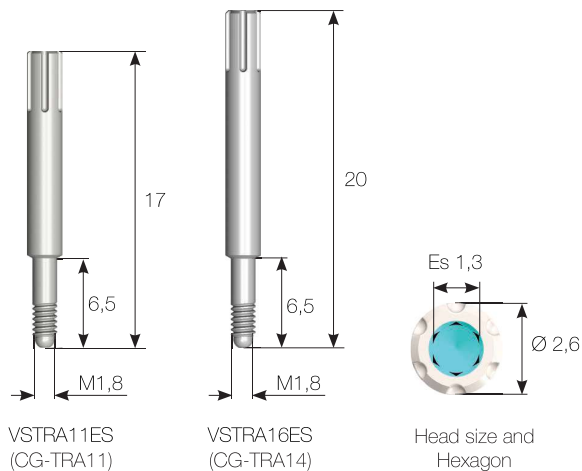


Pick Up screws are made of Gr5 Titanium and come in three different lengths. The length of the screw is associated with the length of the Pick Up.

**Torque:** Tightening to 20-25 Ncm.

**Packaging:** packages include 5 pcs.

# Screws

## For Angled Connector 17°- 30°

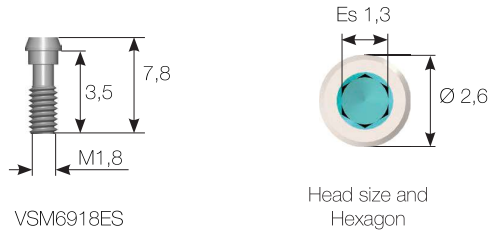


All screws for the Straight or Angled Connector technique are made of Gr5 Titanium.

**Torque for CG-VSM6918 :** Tightening to 25-30 Ncm. **Torque for CG-VSC3414 :** Tightening at 17-20 Ncm.


**Torque for CG-VSTNM :** Tightening at 17-20 Ncm.

**Packaging:** packages include 5 pcs.

## For prosthesis connector 17°- 30° and rightsPer Pick Up

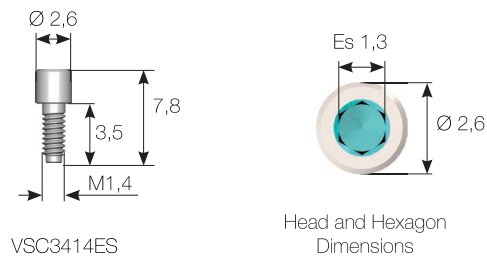

## For Pick Up

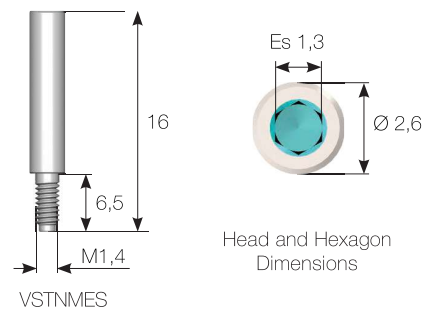

NOTE

[illegible]



**Ornaghi s.r.l.**

Viale Marche, 70 - 20159 Milano (MI)

Phone +39 0392142070

**[www.ornaghimedical.com](http://www.ornaghimedical.com)**



  
MADE IN ITALY