




D3


PuntoZero 3Cones *In* One

CATALOG

Implantline

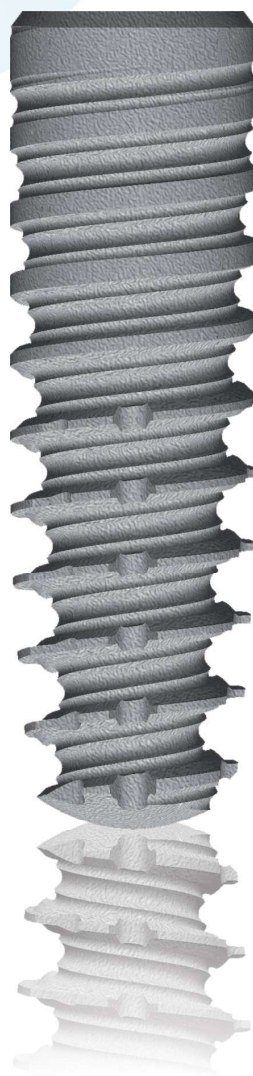

  
ornaghi

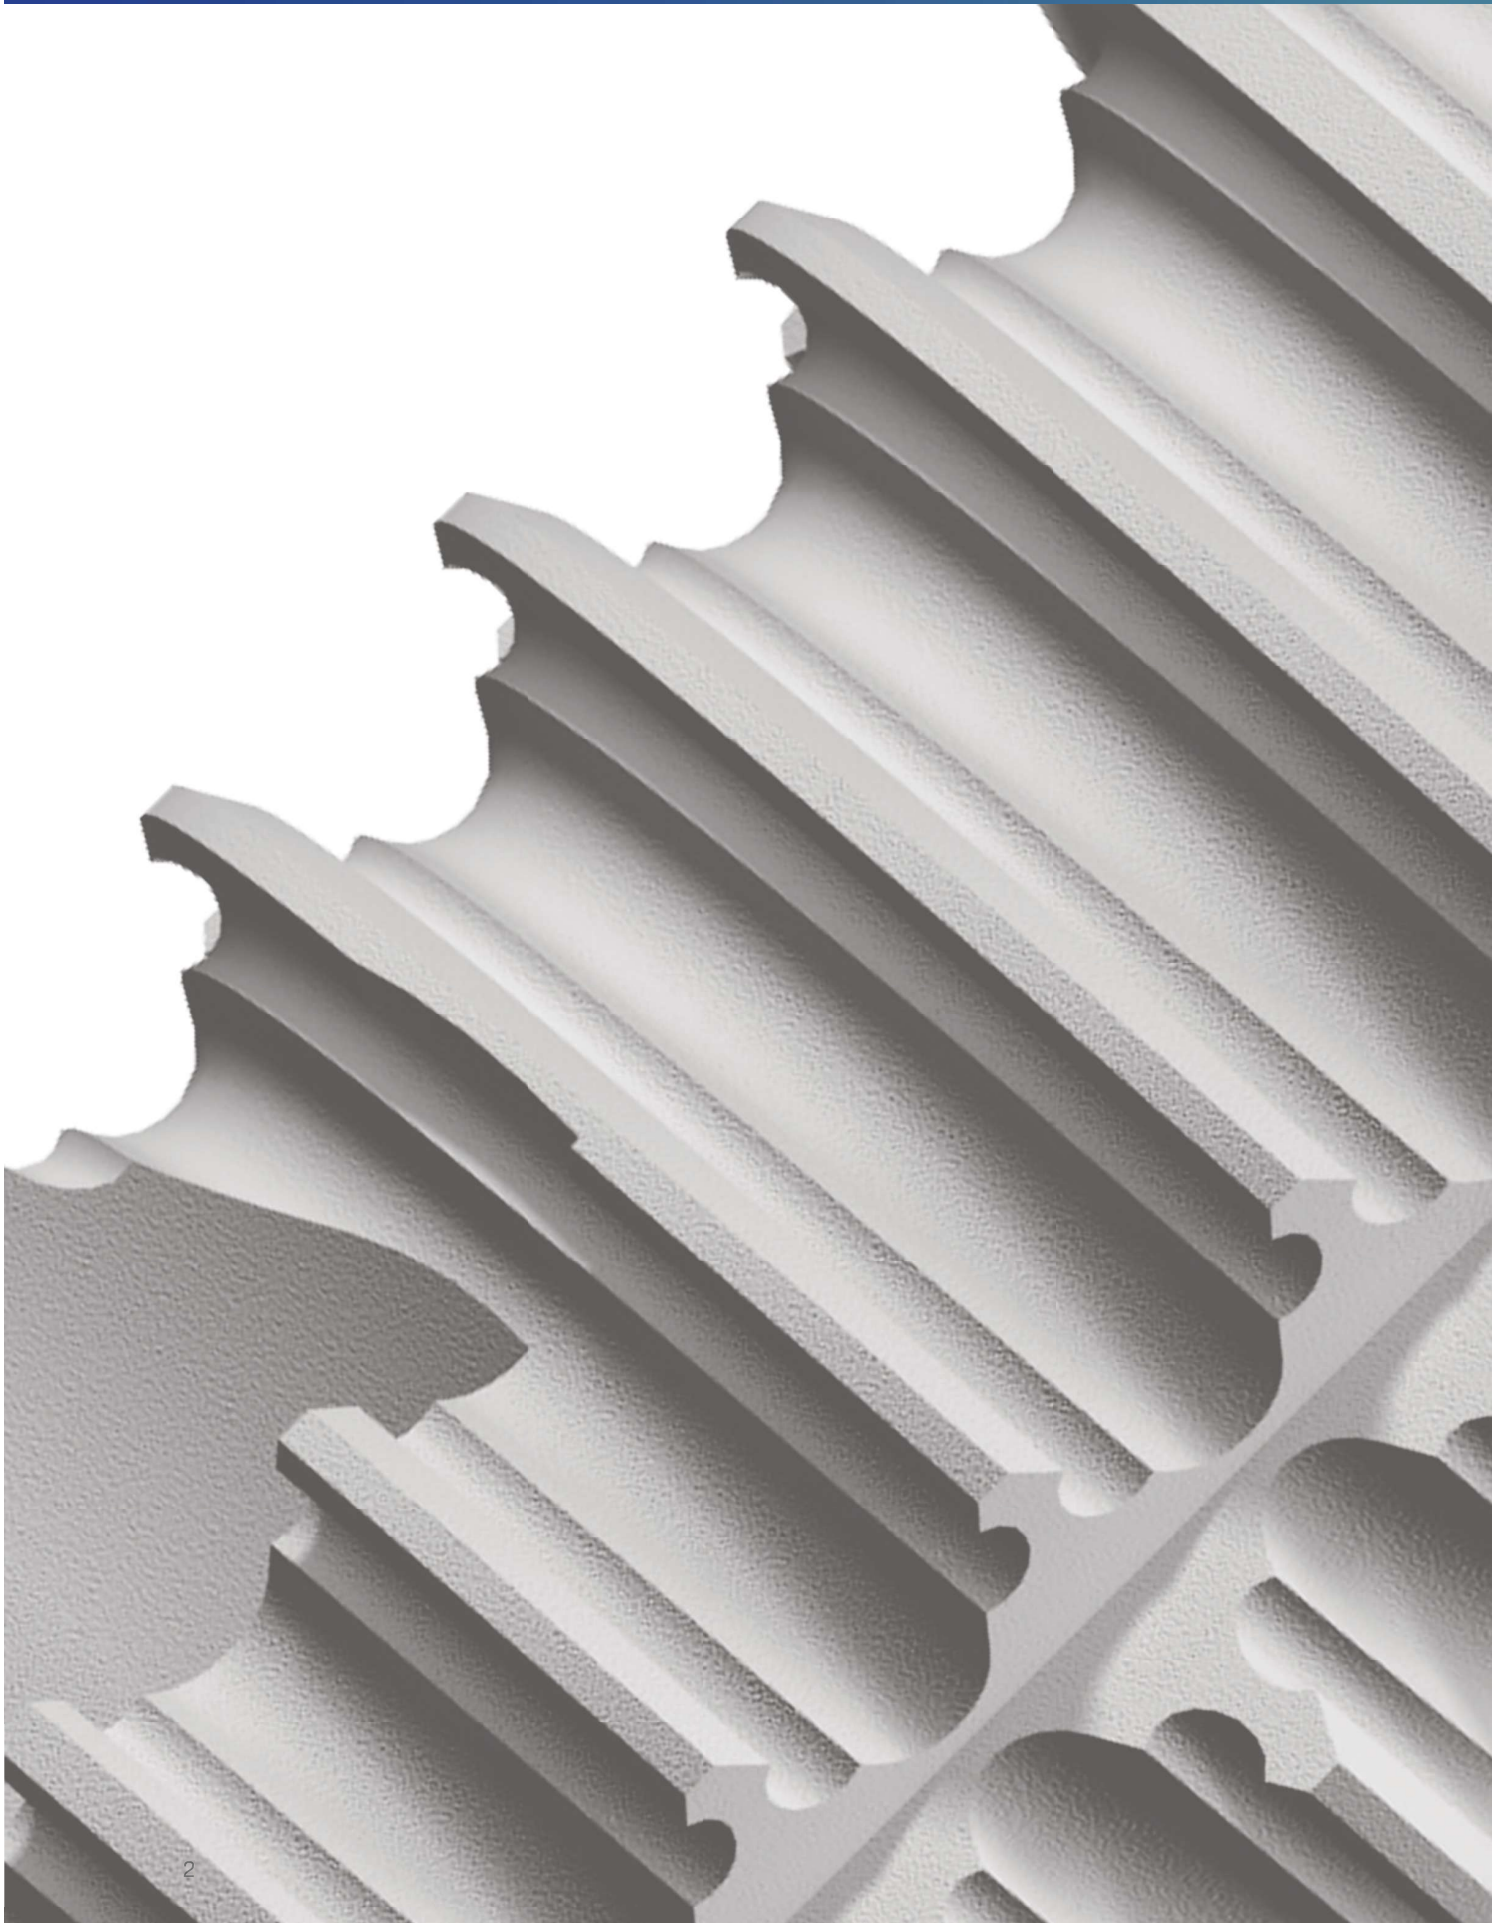


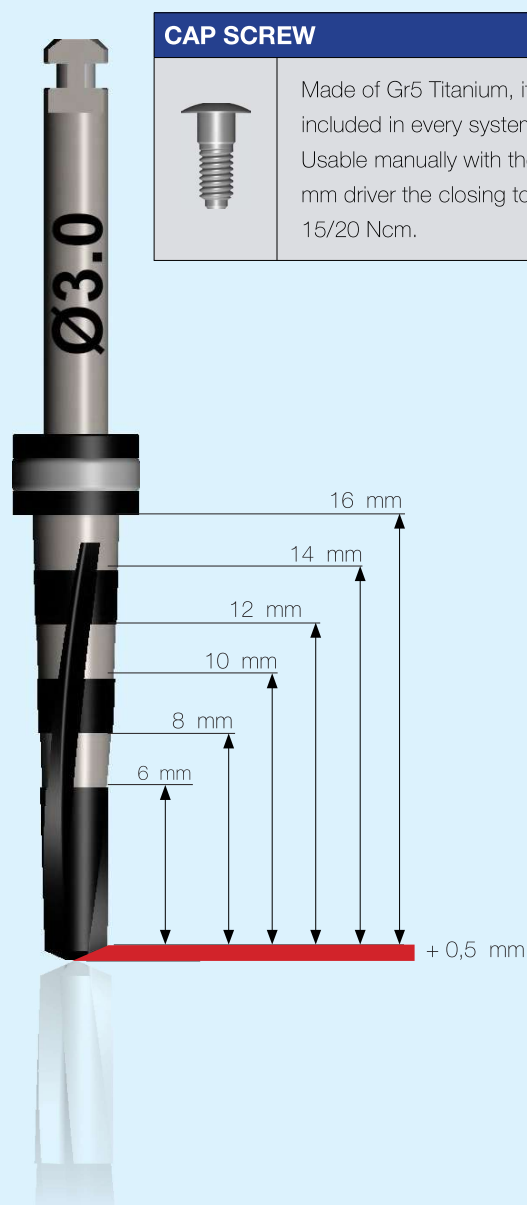
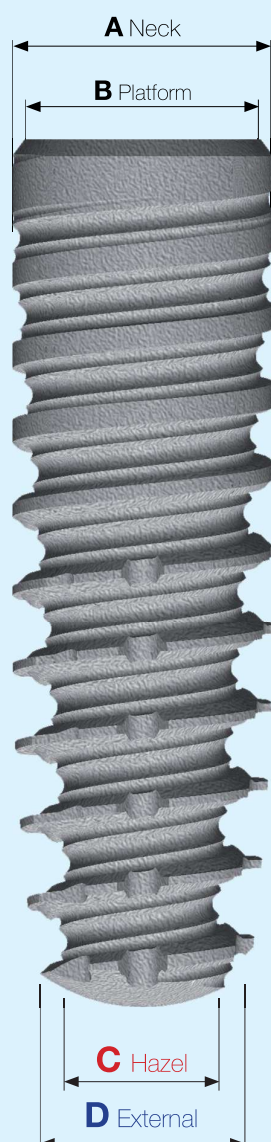
# Contents

The range	4
The surgical sequence	5
Surgical accessories	5
<b>Prosthetic description</b>	
The healing	6
The footprint	7
Prosthetic components	8
Overdenture	9
OT-equator	10
MUA corner abutments	11
Prosthetics for straight MUA	12
TechniqueCAD-CAM Plants	14
TechniqueCAD-CAM IMUA	15
Tightening screws	16
Stop fresa	17

# The range

## Implant

	Length	Art. Code	Size			
			A	B	C	D
 D3.0 Implant	8 mm	CG3008	Ø 3,0	Ø 2,7	Ø 1,15	Ø 2,5
	10 mm	CG3010	Ø 3,0	Ø 2,7	Ø 1,15	Ø 2,5
	12 mm	CG3012	Ø 3,0	Ø 2,7	Ø 1,15	Ø 2,5
	14 mm	CG3014	Ø 3,0	Ø 2,7	Ø 1,15	Ø 2,5



# The surgical **sequence**



IMPLANT Ø 3,0



**Step 1:** Lanceolate bur  
**Step 2:** drill Ø 2,0 - Ø 3,0 implant depth  
**Step 3:** For **DI** drill CS 3,0 h 6 mm

**N rpm:** 900  
**N rpm:** 900  
**N rpm:** 900

## box **contents**

	Size	Art. Code
 lanceolate	-	FBC001
 Cylindrical	Ø 2.0 L16	TDCO216S
 Conical	Imp. Ø 3,0	TDCG30
 Cortical <b>DI</b>	Imp. Ø 3,0	TDCG30
 Screwdriver Implant	L 8 for Imp 3.0	CG-WHD3S
	L 11 for Imp 3.0	CG-WHD3M
 Driver Implant	L 13 for Imp 3.0	CG-DRD3S
	L 17 for Imp 3.0	CG-DRD3M
 Driver Es 1,3	Es 1.3 L 17	DRCO13M
 Screwdriver Es 1,3	Es 1.3 L 10	MNCO13M
 Extractor	Sky blue	CG-CLK02
 Key	25-55 Ncm	CRIC02

# The healing

## Healing abutment




The Healing Abutments **D3.0** are produced in medical grade Gr5 Titanium and are used to condition the soft tissues, preparing them to accommodate the temporary or permanent prosthesis.


**Torque:** Tightening at 15÷20 Ncm.

**Packaging:** The package contains only one Healing abutment.

Ø 3,5

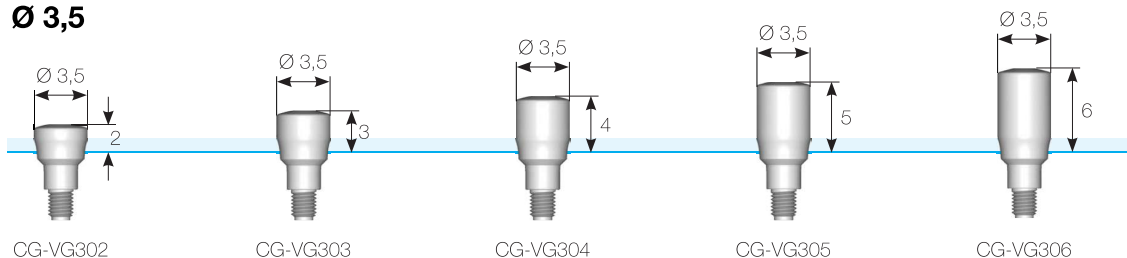


## Healing abutment peek




The Healing abutments peek **D3.0** are produced in medical Peek, they are used to condition the soft tissues preparing them to accommodate the temporary or definitive prosthesis.

**Torque:** Tightening at 20÷25 Ncm.

**Packaging:** the package includes a single Healing abutment peek plus its prosthetic screw.

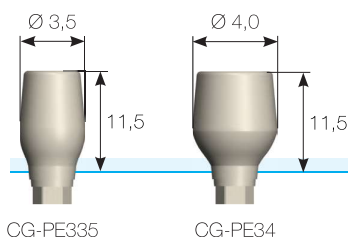

## Temporary titanium abutments




The **D3.0** temporary abutments are made of Gr5 Titanium and are used to condition the soft tissues, preparing them to accommodate the temporary or permanent prosthesis.


**Torque:** Tightening at 20÷25 Ncm.

**Packaging:** the package includes a single temporary abutment plus its prosthetic screw.

With Index

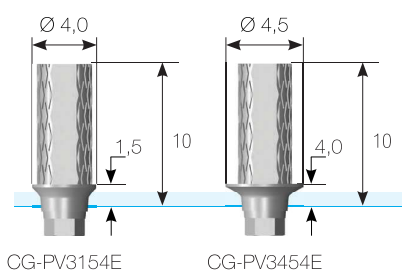


Senza Index

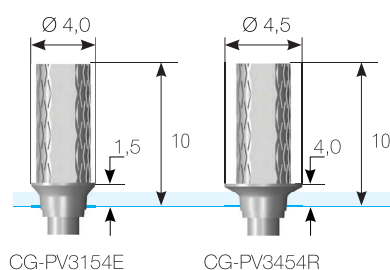

# Theimprint


## Transfer




The **D3.0** impression transfer is made of medical grade Gr5 Titanium and is used to take the impression with an individual tray.

**Torque:** Tightening at 15 Ncm.

**Packaging:** The package includes only one Pick Up and its screw.

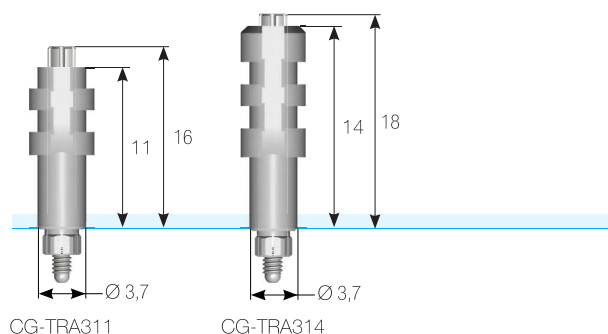

## Analogue




Plaster analogue, inserted in the Pick Up or in the impression Transfer, is used to reproduce the exact position of the implant in the plaster.

**Packaging:** The package contains only one Plaster Analogue.

# Prosthetic components


## Straight stumps to finish




All straight and angled **D3.0** Titanium Abutments are produced in Gr5 Titanium and are used to create the definitive prosthesis.

**Torque:** Tightening at 20÷25 Ncm.

**Packaging:** the package includes the titanium abutment, one laboratory screw and one patient screw.

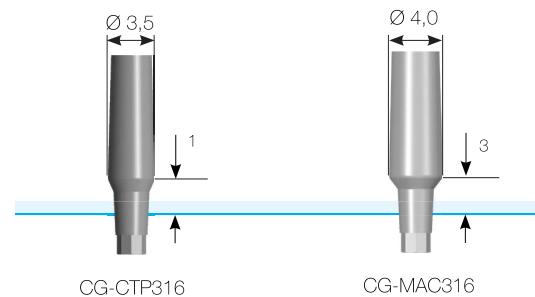


## Angled Stumps




All straight and angled **D3.0** Titanium Abutments are produced in Gr5 Titanium and are used to create the definitive prosthesis.

**Torque:** Tightening at 20÷25 Ncm.

**Packaging:** the package includes the titanium abutment, one laboratory screw and one patient screw.

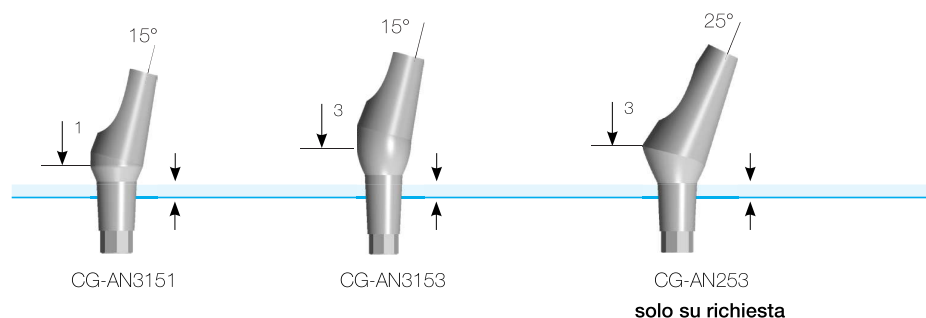


## Castable abutments with Chrome Cobalt base



The Castable Abutment has a base made of **Cobalt Chrome** and is used to create the definitive prosthesis by overcasting.

**Torque:** Tightening at 20÷25 Ncm.

**Packaging:** the package includes a castable, a Chrome Cobalt base, a laboratory screw, a patient screw.

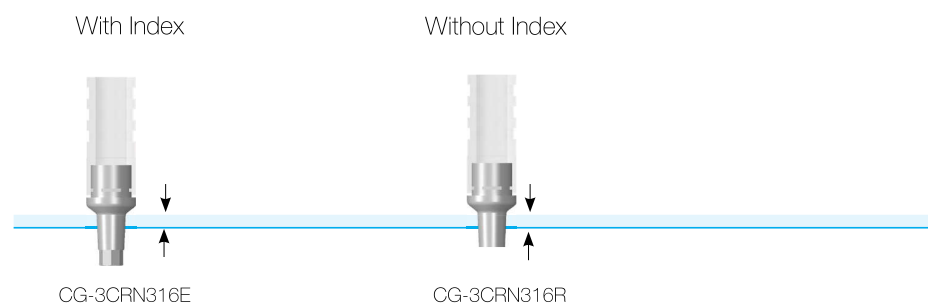



# Overdenture


## Ball abutment



The Ball Abutment **D3.0** in Titanium Gr5. It is used to make removable prostheses.


**Torque:** Tightening at 25 Ncm.

**Packaging:** The package contains only one Ball Abutment.

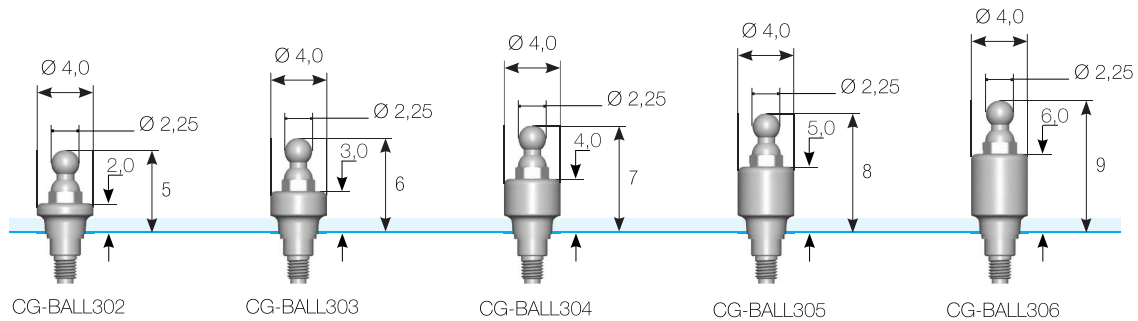

## Ball Abutment Spare Parts

O-Ring Seal



CG-GO01

Kit Package



1 pz.

3 pz.


Pack of 5 pcs.  
O'Ring



ORCO01

standard estate

O-Ring Seal



CG-GO02

Kit Package



1 pc.

3 pcs.

Pack of 5 pcs.  
O'Ring




ORCO02

soft hold

## Overdenture Spare Parts

Container




CG-CA001

Standard sealing sheaths




CA001

Soft sealing sheaths



CN001

Standard sealing sheaths



CN002

# Ot equator

## Ot Equator kit




The Ot Equator component is made of Gr5 titanium and coated in Tin.

**Torque:** Tightening at 25 Ncm.


### La confezione prevede:

Titanium attachment coated in Tin, 1 Stainless steel container for caps, 1 Protective disk, 4 Assorted caps (1 extra-soft, 1 soft, 1 standard, 1 strong).

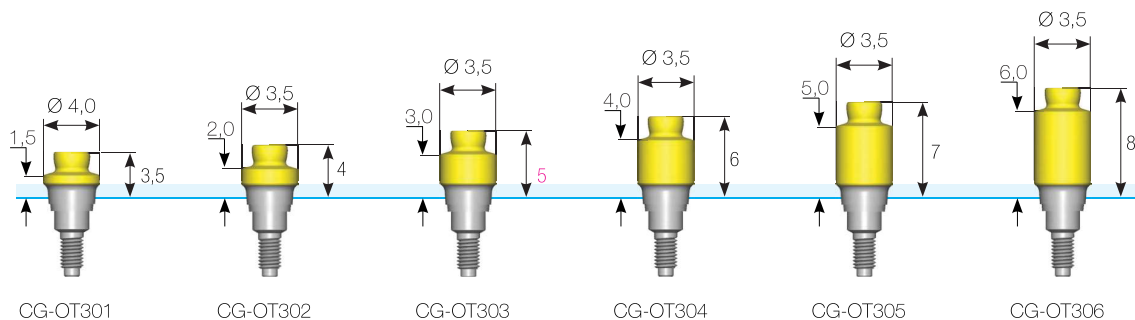


## Overdenture Spare Parts

### Sheaths




CG-CNL4

From the laboratory




CG-CBST4

Standard hold (1.8 Kg)




CG-CRS4

Soft hold (1.2 Kg)



CG-CGE4


Extra soft hold (0.6 kg)



CG-CVF4


Strong Hold (2.7 Kg)

## Container



CG-C12

## Protective sheath



GACG001

## Ot Equator Laboratory

Plaster analogue



CG.ANSF01

Individual Transfer



Ref. 144MTE

Tear-off transfer



Ref. 044CAIN

# MUA**angled**abutments


## Straight connectors




The straight connector is made of Gr5 titanium and is used to create prostheses screwed onto multiple elements and in the case of disparallel implants (all on four technique).

**Torque:** Tightening at 25 Ncm.

**Packaging:** The packaging contains a single component.

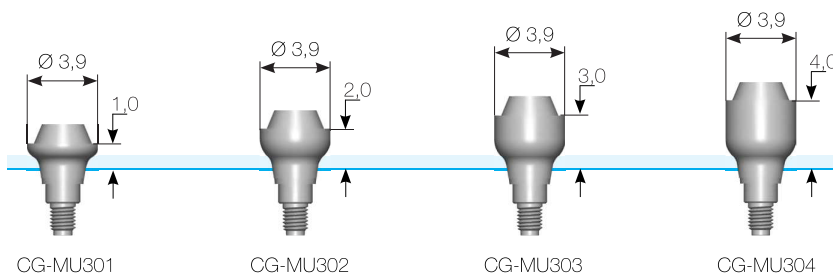

## Cover for Standard and Angled Connectors




CG-VGSMU3

The healing cover for straight connector and angled connector is made of Gr5 titanium and serves to protect the connection cones of straight connectors and angled connectors.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package includes a healing cover and its screw.


## MUA Driver Accessory

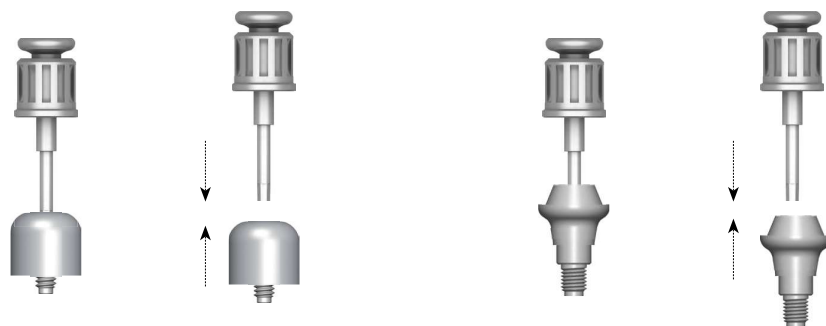

The accessory to use to screw the MUA healing and the MUA is the 1.3 hex driver that is used for prosthetic screws.

# Prosthetics for **straight** MUA

## Straight titanium abutment

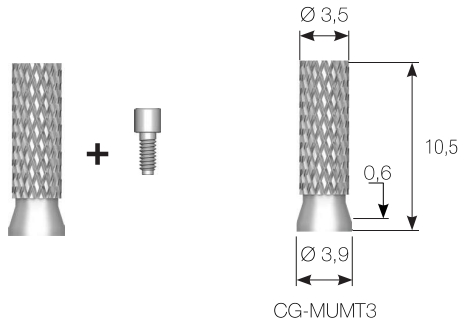


The Titanium Abutment for straight and angled connector **D3.0** It is produced in Gr5 Titanium and is used to create temporary and/or permanent prostheses.

**Torque:** Tightening at 20 Ncm.

**Packaging:** the package includes a single Titanium Abutment with a prosthetic screw.

## Calcinable abutment

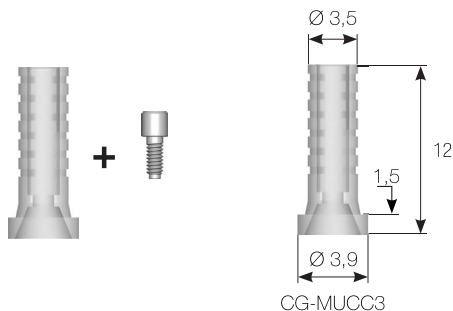


The Castable for straight and angled connectors **D3.0** is made of PMMA and is used to cast metal.

**Melting range °C :** 160-175

**Torque:** Tightening at 25 Ncm.

**Packaging:** The package includes a castable, a prosthetic screw.

## Footprint Pick Up

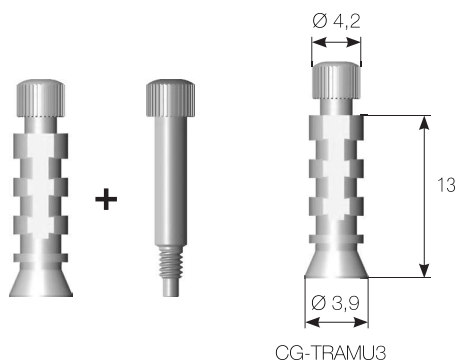


The Pick Up for straight and angled connectors **D3.0** is made of Titanium Gr5 and is used for taking impressions with an individual tray.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package includes a castable, a screw.

## Plaster analogue

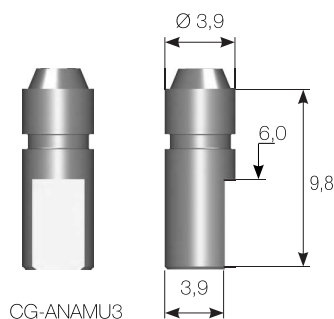

The plaster analogue is the same as that used for the CAD/CAM technique, it is made of Gr5 titanium.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package contains only one analogue.

# CADCAM Technique


## Scan Marker by Implant



The Marker is produced in a single piece of Gr5 Titanium.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package includes a Marker and a screw for its tightening CG-VS7818.

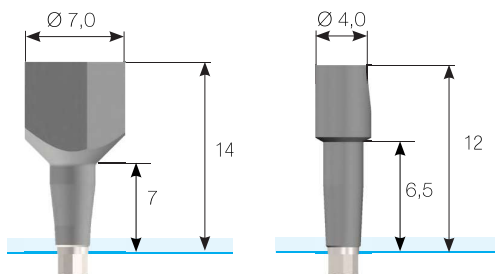

CG-SB303


CG-SB301SLIM

The Marker is produced in a single piece of Gr5 Titanium.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package includes a Marker and a screw for its tightening CG-VS7818.

## CAD CAM Premilled for cementation

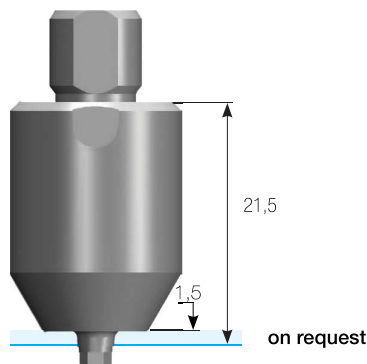


CG-MCU301

The premilled are produced in titanium Gr5, a single diameter and height. The Premilled diameter 10 mm is ideal for customised processing on milling machines.

**Torque:** Tightening at 25-30 Ncm.

**Packaging:** The package includes a Premilled and a screw for tightening it.

## Digital analogue for CAD CAM technique



M1,6  
CG-ANCD03


The digital analog for the CAD CAM technique is made of Gr5 titanium. Its particular shape allows for easy positioning in the printed models and its anchoring to the model with considerable simplicity thanks to the use of a screw (M1.6) that is screwed between the bottom of the model and the lower part of the analog.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The packaging includes an analogue with the screw.

# CAD**CAM**Technique

## You Bonding Base for CAD/CAM Technique




The Ti base for bonding are made of Gr5 titanium. The Ti base are offered with three different heights to compensate even for deep mucosal tracts.

**Torque:** Tightening at 25-30 Ncm.


**Packaging:** The package includes a Digital Ti base and a CG-VS7818 prosthetic screw.

With Index      Without Index




CGTBE30      CGTBR30

With Index      Without Index



CGBTE32      CGTBR32


With Index      Without Index

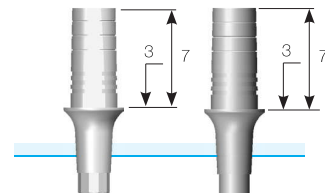

CGTBE33      CGTBR33

# CADCAM MUA Technique


## MUA scan marker



The MUA Abutment Marker is made of Gr5 Titanium.


**Torque:** Tightening at 15-20 Ncm.

**Packaging:** The package includes a Marker and a screw for its tightening CG-VS3414.



CG-SB03


## Digital Ti base MUA



The Ti base for MUA is made of Gr5 titanium.

**Torque:** Tightening at 25-30 Ncm.

**Packaging:** The package includes a Digital Ti base and a CGVS3414 prosthetic screw.

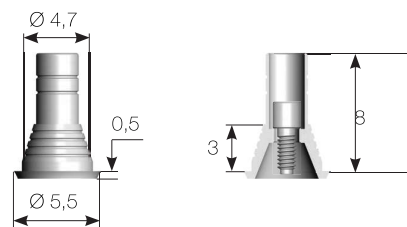

CGTBMU301

## Digital analogue for CAD CAM technique




The digital analog MUA for the CAD CAM technique is made of titanium Gr5. Its particular shape allows for easy positioning in the printed models and with considerable simplicity its anchoring to the model thanks to the use of a screw (M1.6) that is screwed between the bottom of the model and the lower part of the analog.

**Torque:** Tightening at 15-20 Ncm.


**Packaging:** The packaging includes an analogue with the screw.

# Screw

## For standard stumps



CG-VS300



CG-VS300L  
(LABORATORY)

The prosthetic screws are made of Titanium Gr5 and are of two types. The **D3.0** system includes a fuchsia colored screw for laboratory use and a gray screw to be used only for the patient.

**Torque:** Tightening at 20-25 Ncm.

**Packaging:** packs contain 5 pcs.

## For pick up imprint



CG-TVSRA311



CG-VSTRA314

## For Body scan



VSCG16SB-D3


The Pick Up screws are made of Titanium Gr5 and are of two different lengths. The length of the screw is associated with the length of the Pick Up.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** packs contain 5 pcs.

# MUA prosthetic screws

## For pick up 0° footprint




CG-VSTNM3

The MUA Pick Up screw is made of Gr5 Titanium.

**Torque:** Tightening at 15-20 Ncm.

**Packaging:** packs contain 5 pcs.

## For temporary and castable abutment MUA



VSCC0265

The MUA prosthetic screw is made of Gr5 Titanium.


**Torque:** Tightening at 20-25 Ncm.

**Packaging:** packs contain 5 pcs.




# Stop-fresa

The stops for the Ø 2.0 cutter

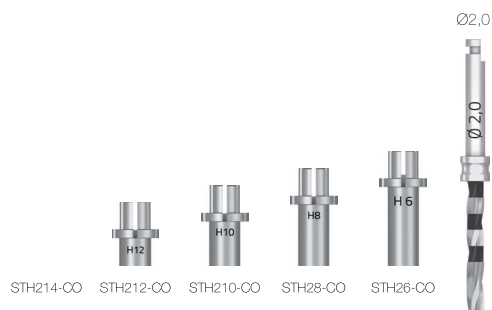


The stops for the cutter Ø 3.0 - Ø 3.3

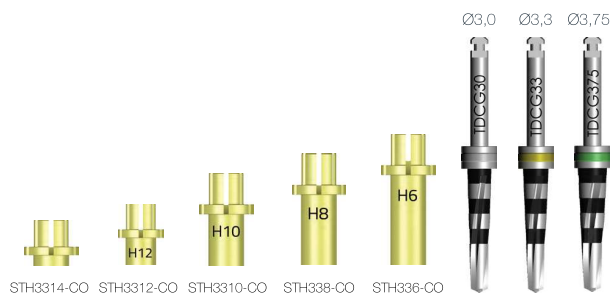

The stops for the cutter Ø 3.75 - Ø 4.2



The stops for the cutter Ø 5.0 - Ø 6.0

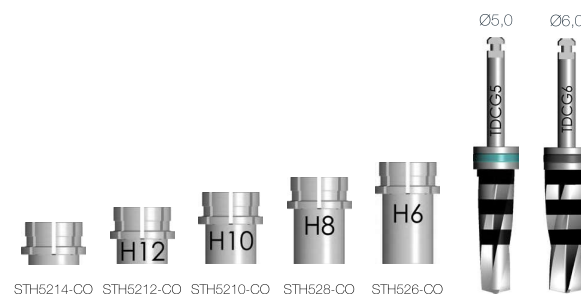


## The cutter stops

Are made of Ti Gr5, their use is foreseen on all **D3.0** cutters. The depth that the stop can reach is laser engraved on the body of the cutter stop (Fig.01). The cutter stop is fixed to the cutter by means of a mechanical seal. By orienting the cut cylindrical part upwards, the cutter tip engages downwards, in this way the cutter and the stop are assembled (Fig.02).

## The cutter stop box

The cutter stop box is designed to make it easy to apply and remove the stop from the cutter, without having to touch the accessories with your hands.

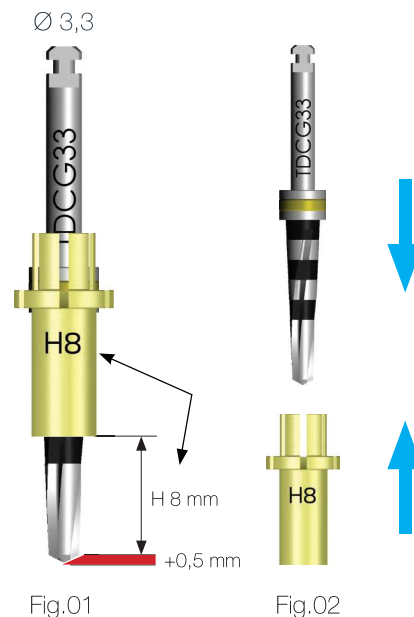

Code	Description
KIT-STCO	COMPLETE 20 STOPS
-	SINGLE STOPS



KIT-STCO

## NOTE

[illegible]

## NOTE

[illegible]



**Ornaghi s.r.l.**

Viale Marche, 70 - 20159 Milano (MI)

Phone +39 0392142070

**[www.ornaghimedical.com](http://www.ornaghimedical.com)**



  
MADE IN ITALY